

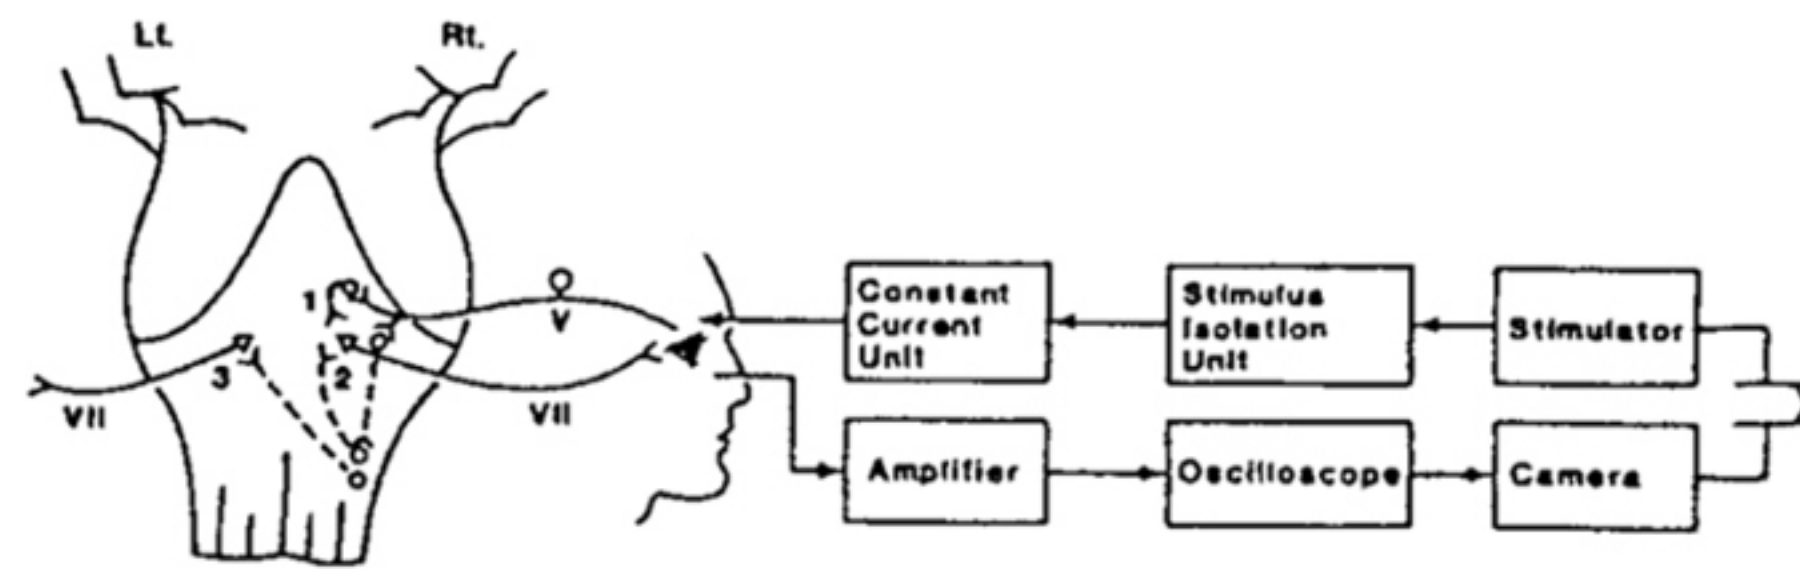
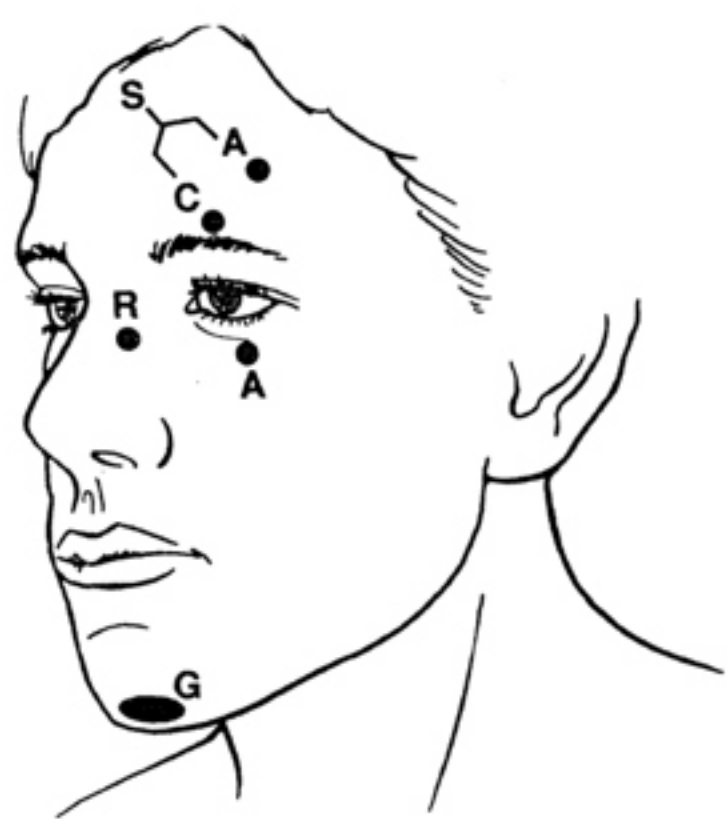




BLINK REFLEX - ODRUCH MRUGANIA

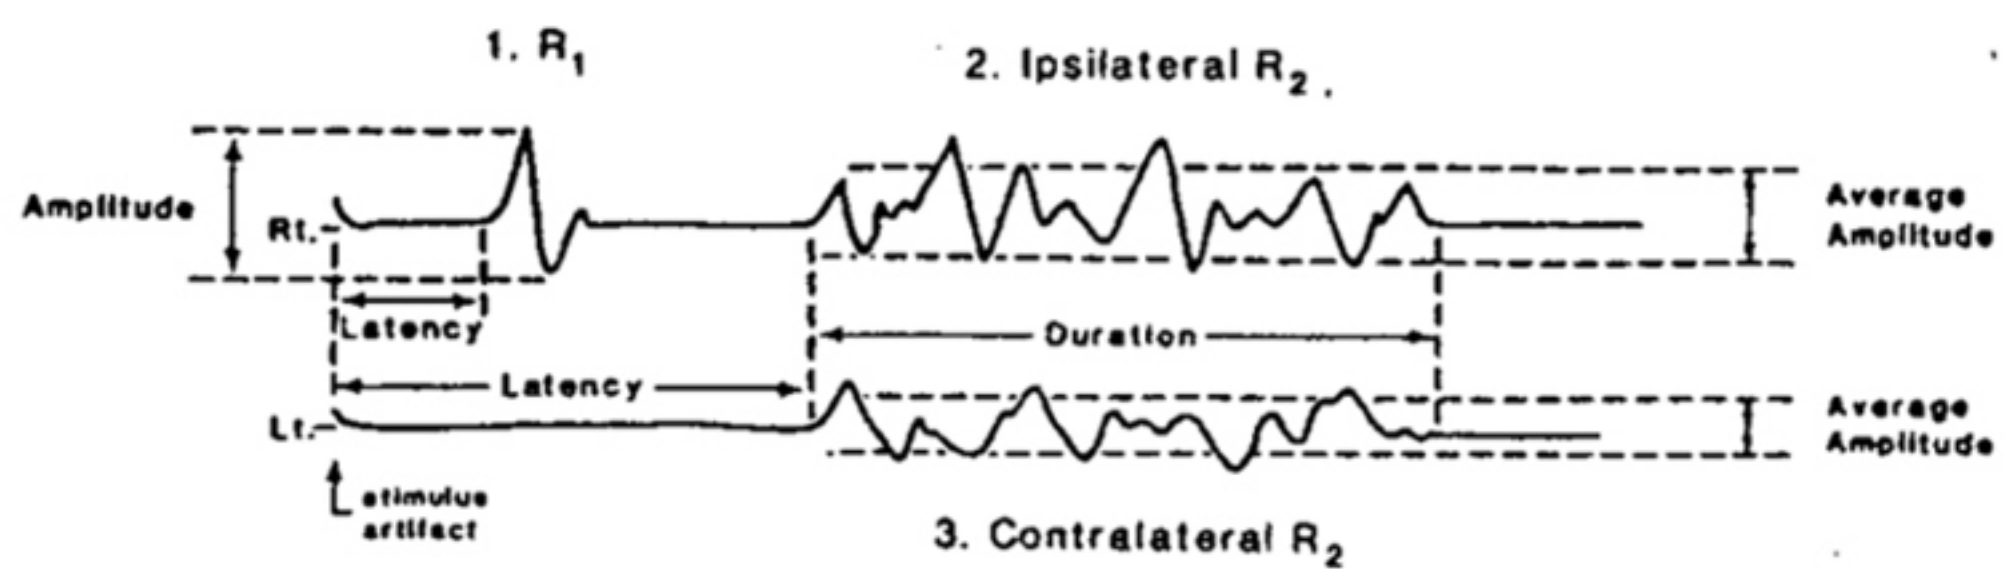

FACIAL NERVE - NERW TWARZOWY

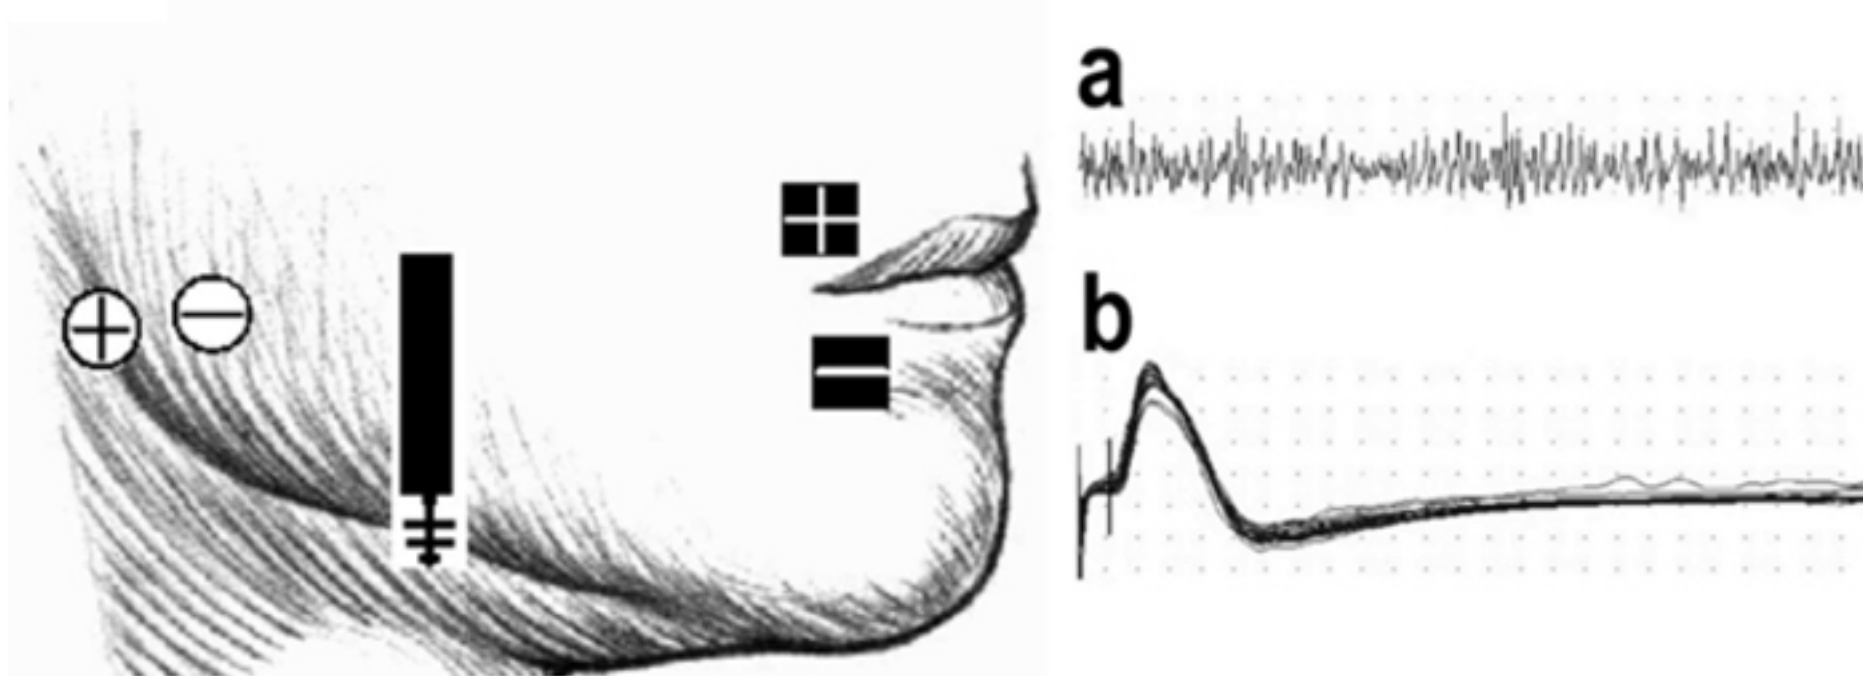

TEST MIASTENICZNY - DECREMENT

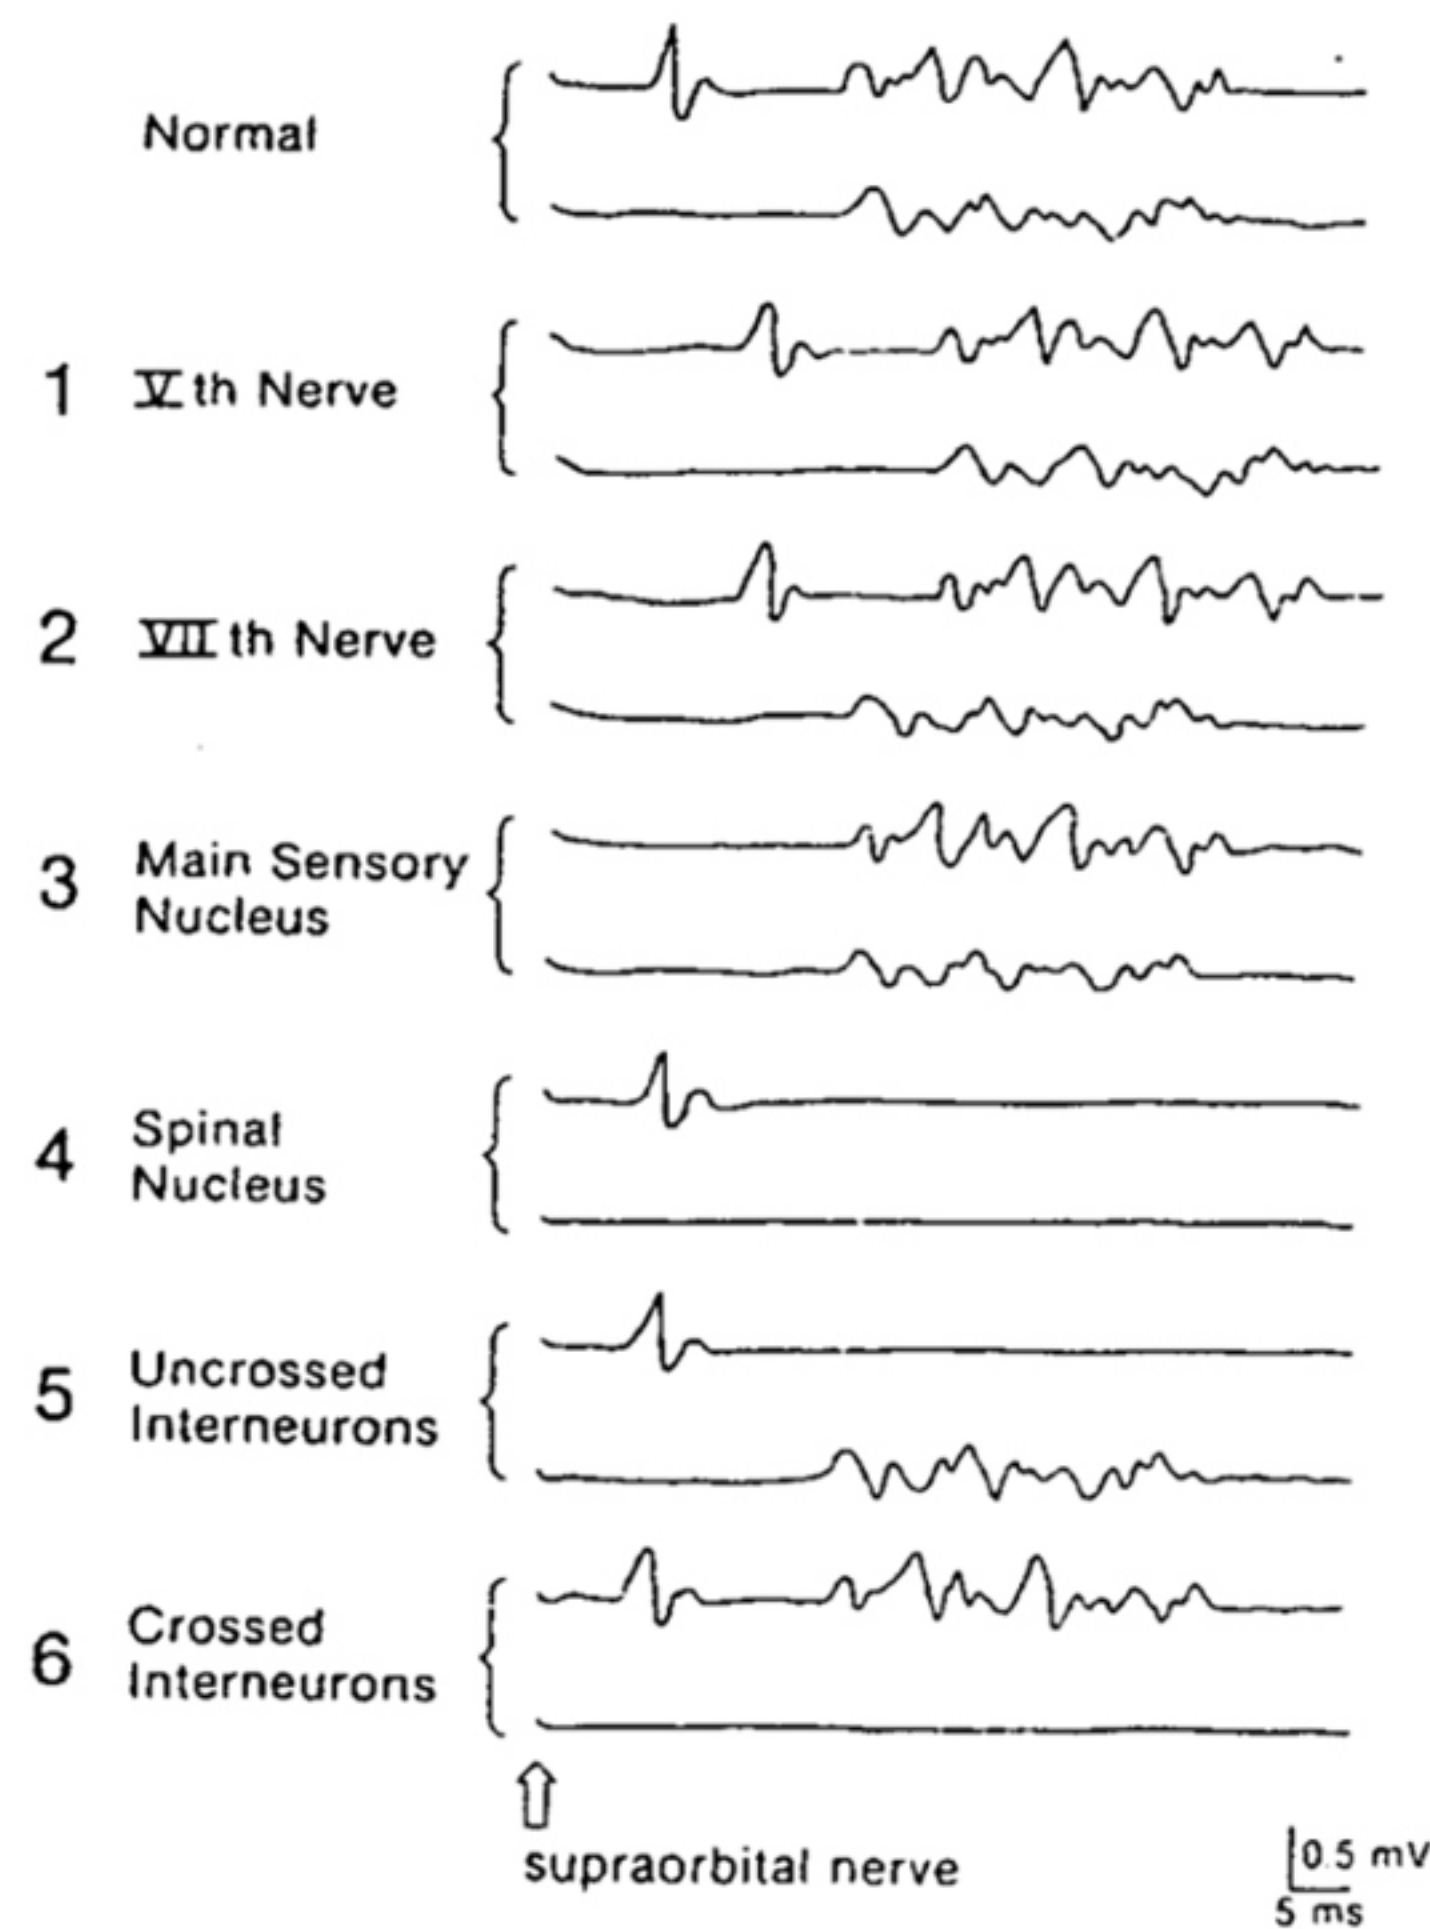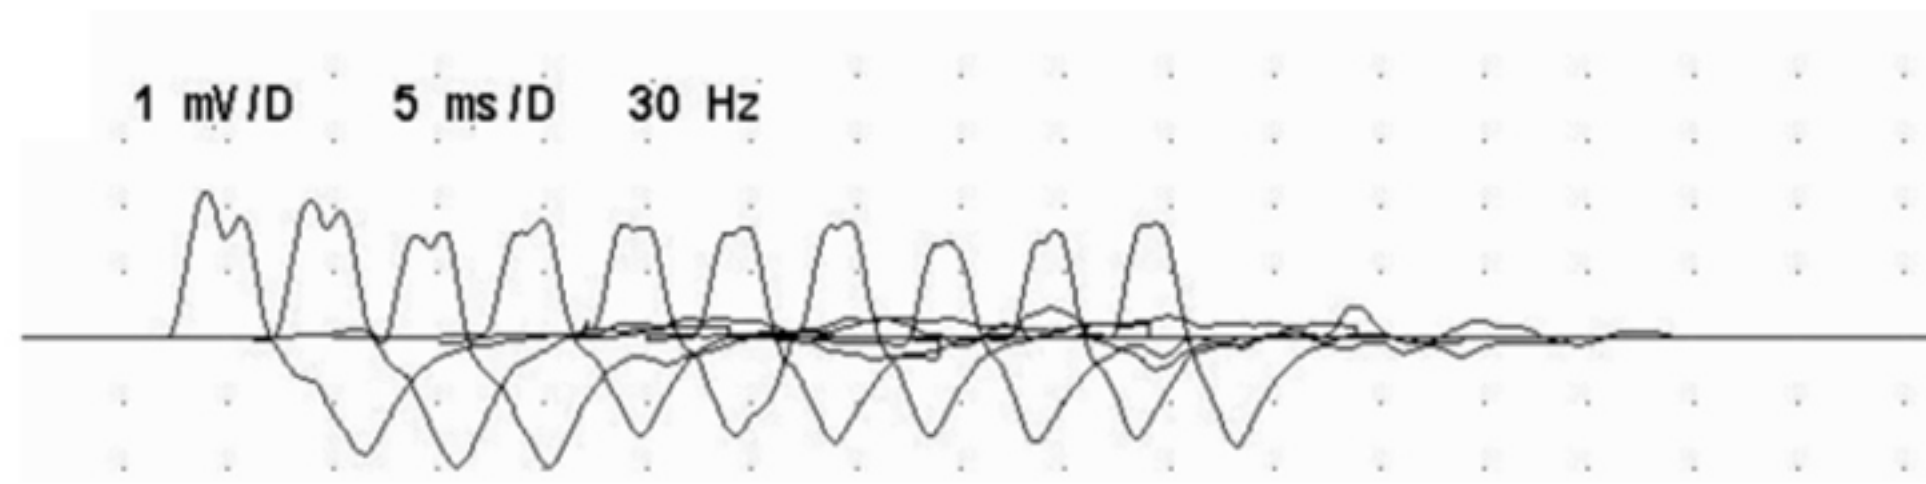

SSR

Data on results from SSR examinations during recordings from upper and lower extremities following all three applied types of stimuli. Ranges, means and standard deviations are shown.

Parameters	Upper extremities recordings (N=40)	Lower extremities recordings (N=40)
Electrical stimulation		
Amplitude (mV)	0.19-2.36 1.13±0.58	0.12-2.00 0.73±0.52
Latency (s)	1.31-1.89 1.58±0.16	1.75-2.72 2.13±0.21
Area (mV/s)	0.22-4.18 1.38±0.81	0.11-3.10 0.87±0.65
Sound stimulation		
Amplitude (mV)	0.12-3.40 0.99±0.89	0.14-3.01 0.56±0.51
Latency (s)	1.15-1.94 1.56±0.23	1.27-2.64 2.09±0.28
Area (mV/s)	0.19-4.72 1.14±1.08	0.13-3.61 0.66±0.68
Electrical and sound stimulation		
Amplitude (mV)	0.20-2.24 1.15±0.60	0.09-3.06 0.71±0.58
Latency (s)	1.18-1.80 1.51±0.14	1.65-2.61 2.09±0.24
Area (mV/s)	0.22-5.32 1.44±0.92	0.09-3.83 0.84±0.71

